

FIG. 1A

102290-95676860

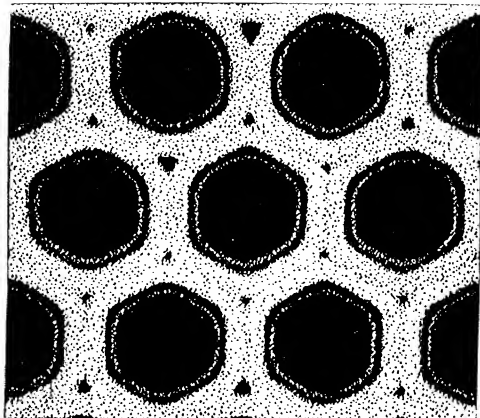


FIG. 1B

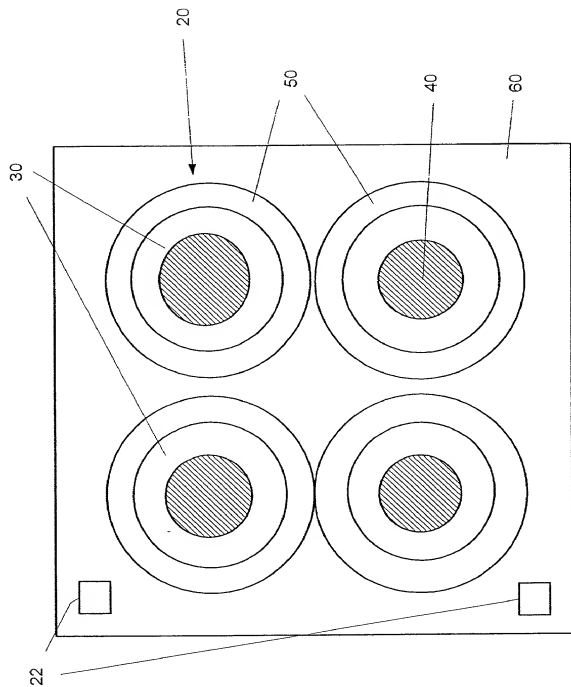


FIG. 2

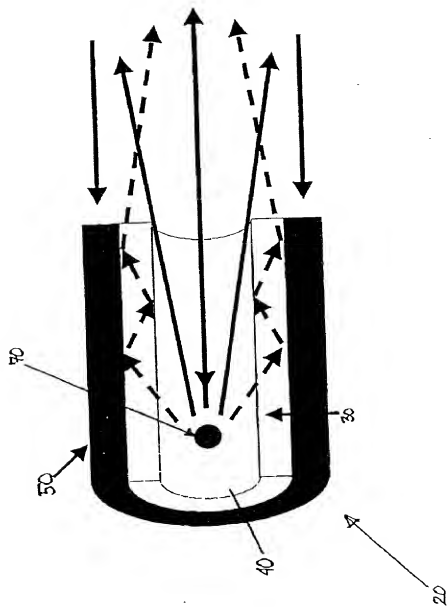


FIG. 3


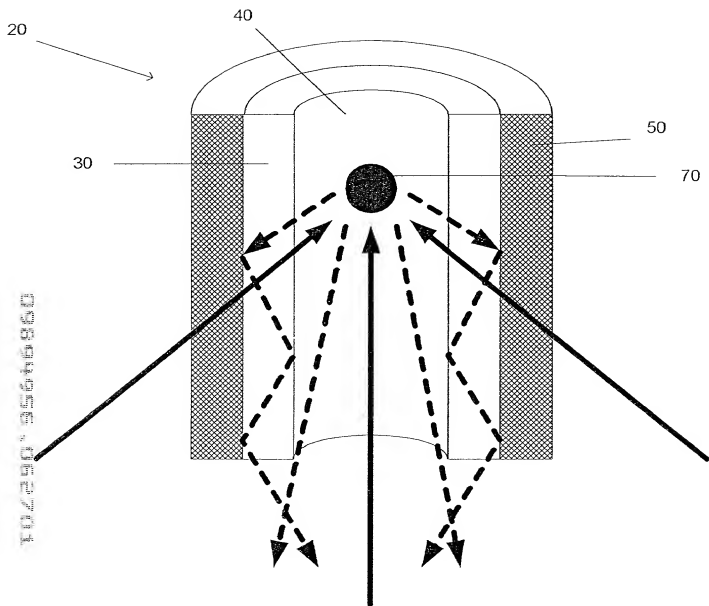


FIG. 4

Wicking



100

Humidified Incubation



Imaging &
Recovery



FIG. 5

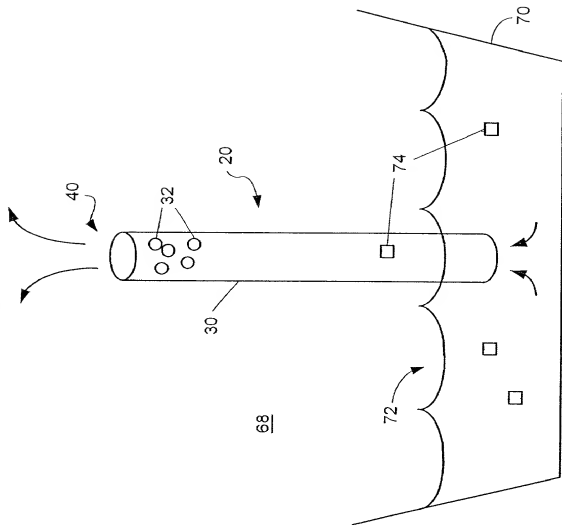


FIG. 6

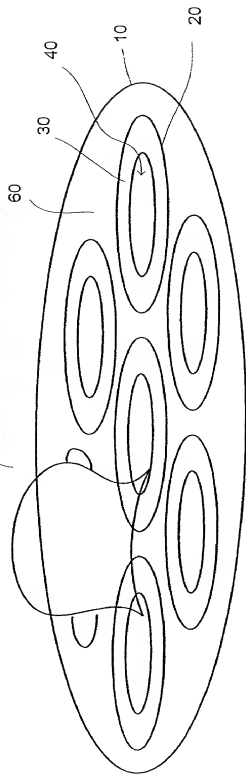


FIG. 7A



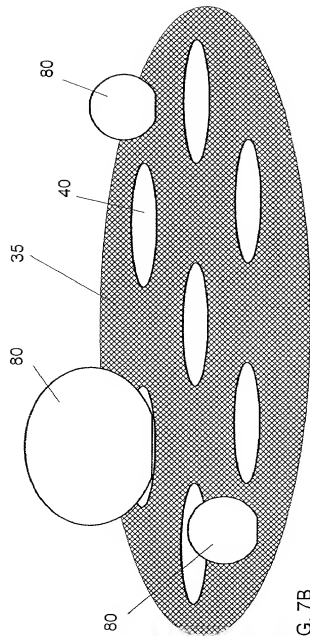



FIG. 7B

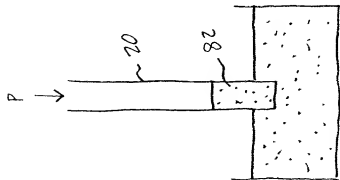

A.



B.

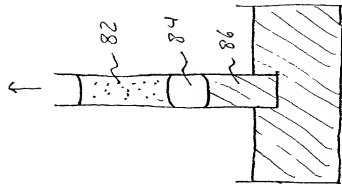

C.

FIG. 8

capillary array.

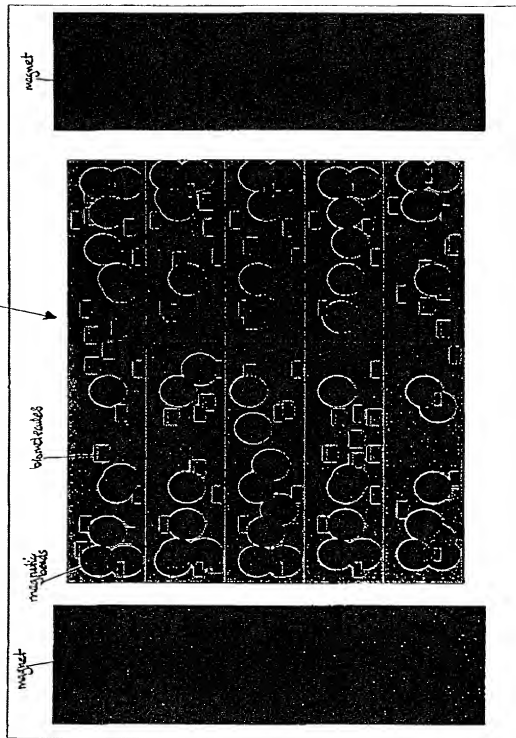
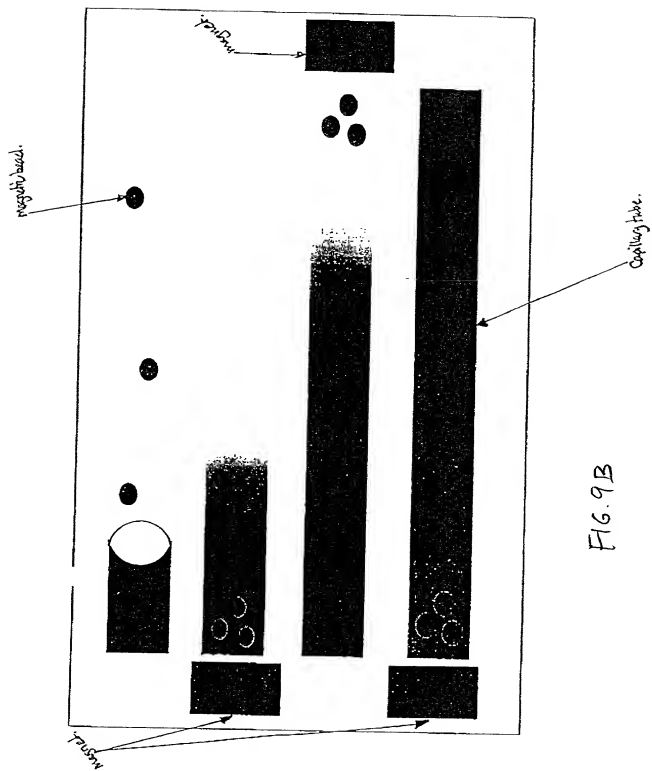


FIG. 9A

[illegible]


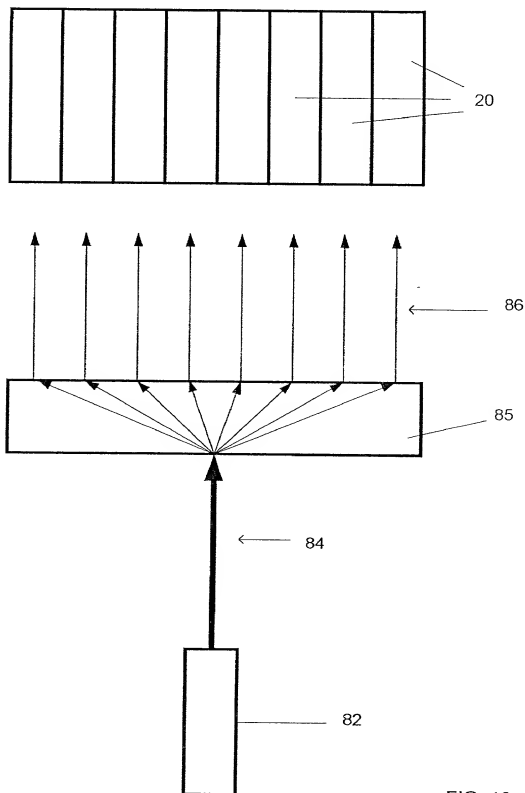


FIG. 10


Automated Hit Detection & Recovery System

FIG. 11

100

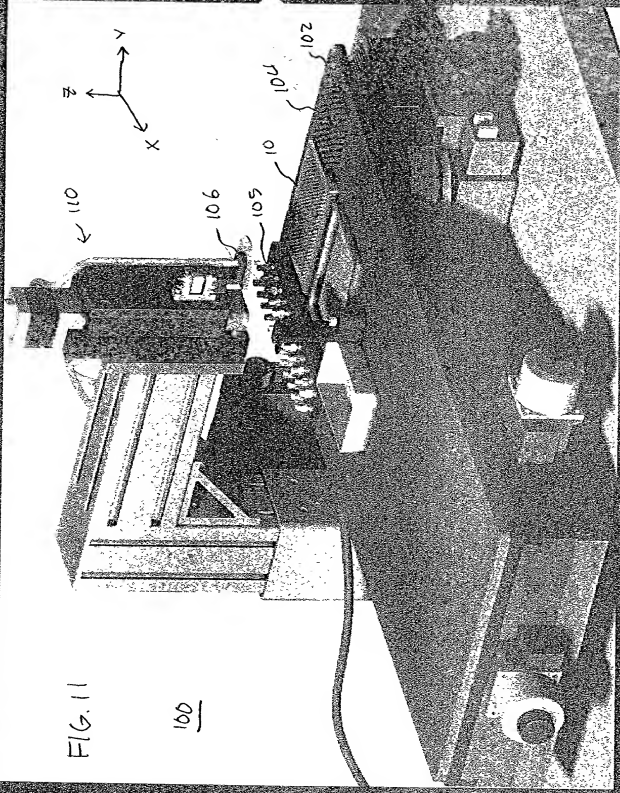

09394956.062701

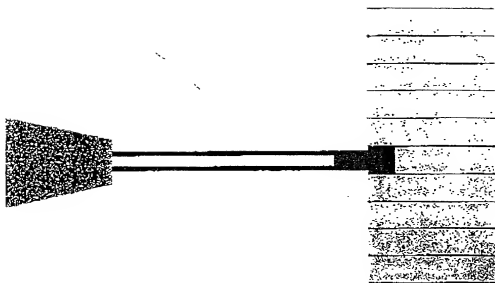

B



A

FIG. 12

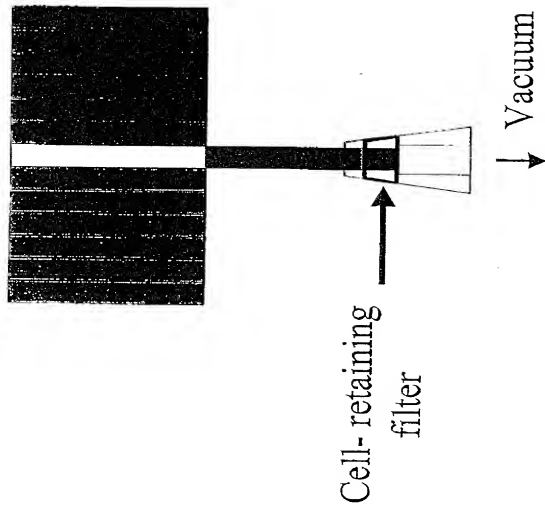


FIG. 12C

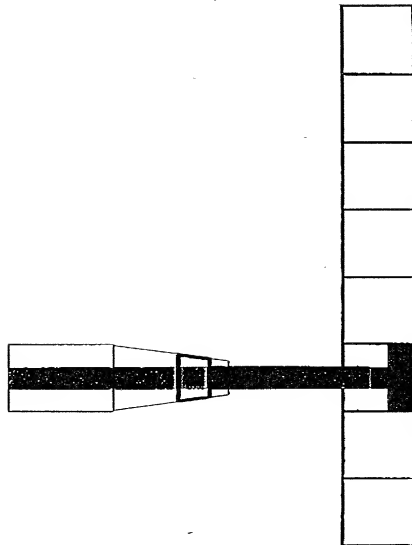


FIG. 12 D